


Simplifying wound healing Wound Infection Pathway

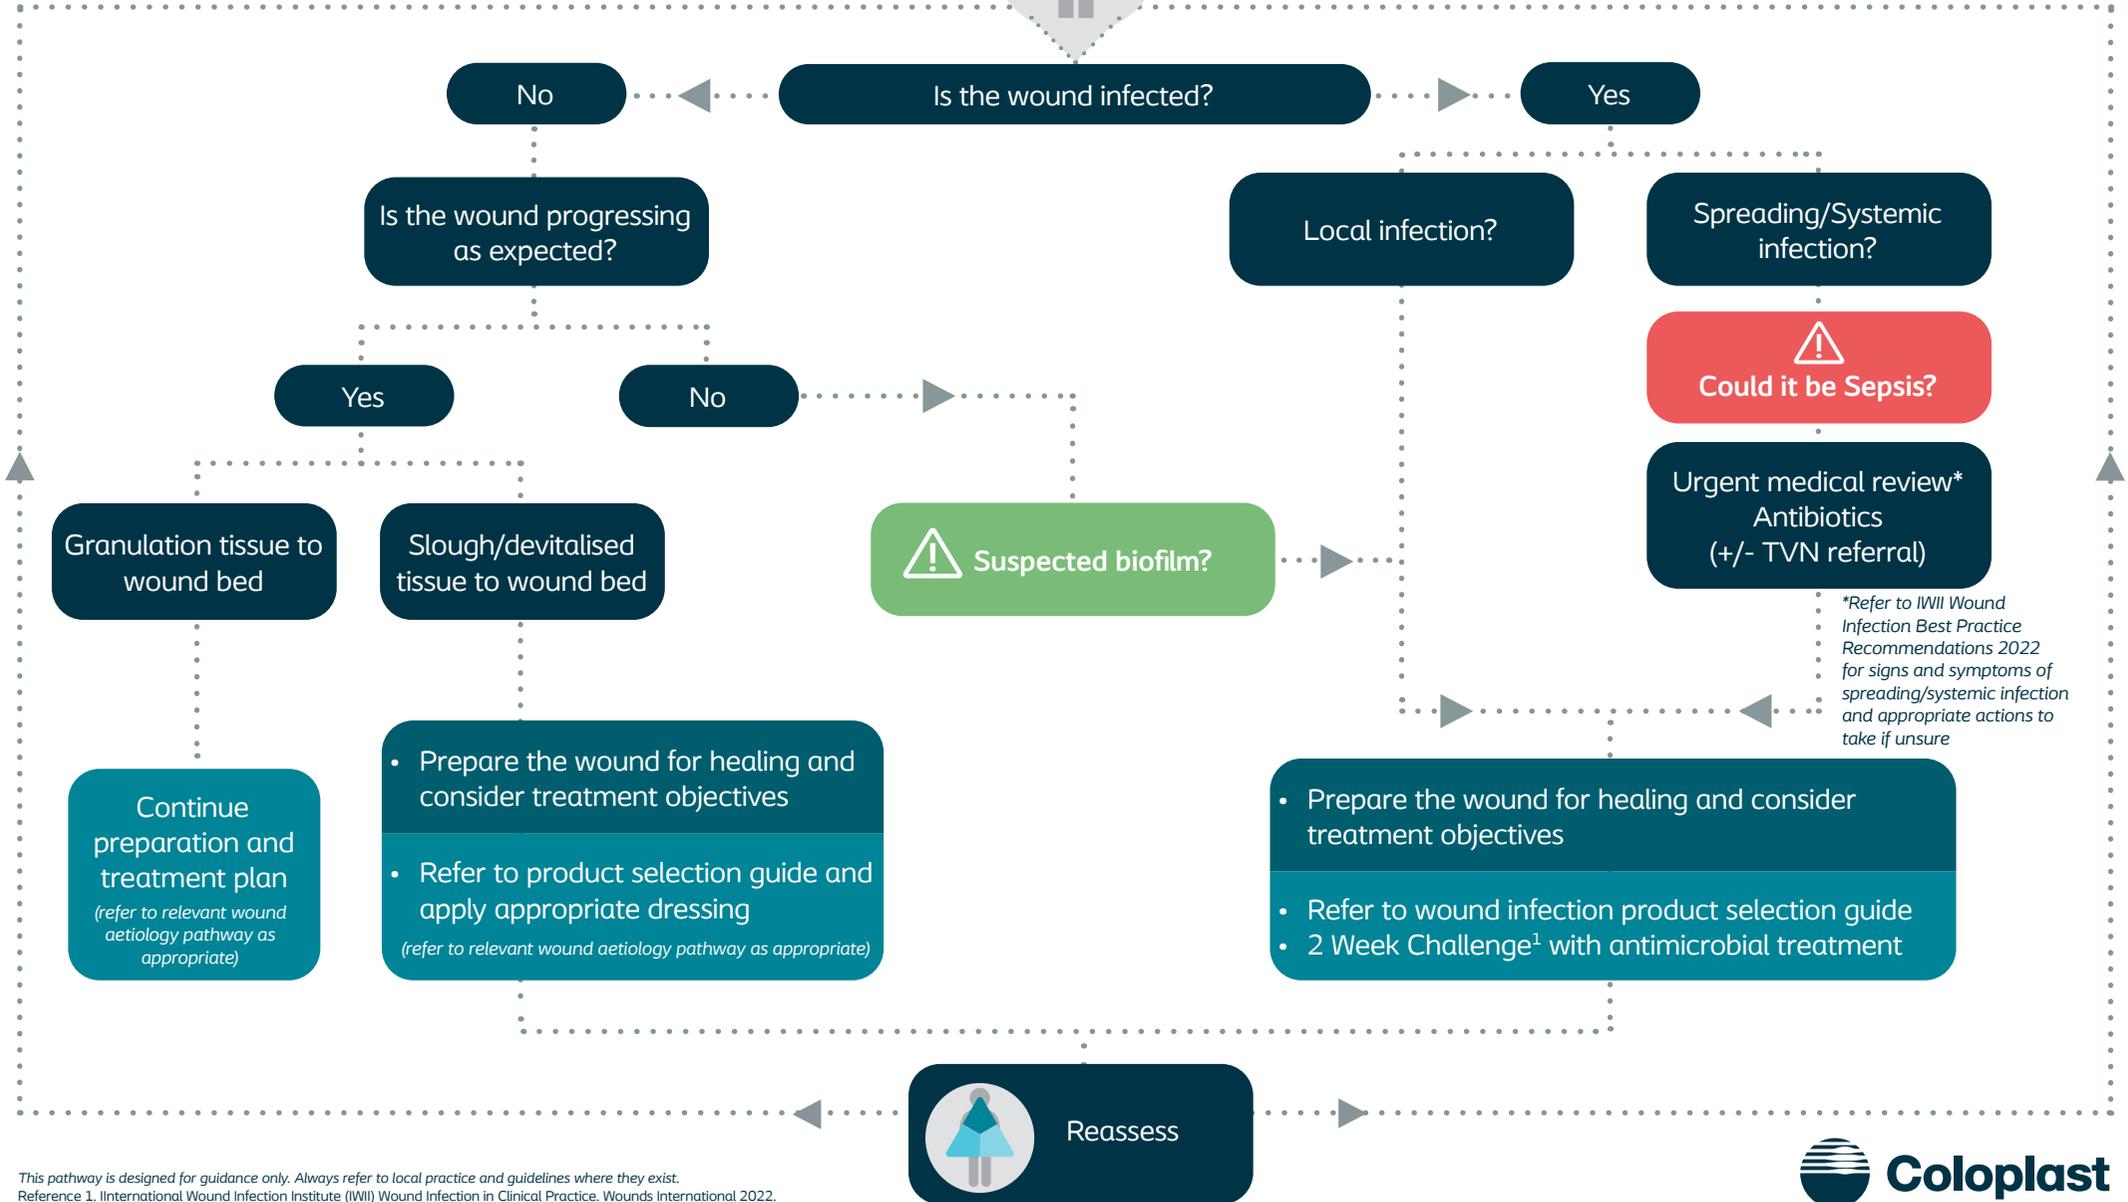

This pathway is designed for guidance only. Always refer to local practice and guidelines where they exist.
Reference 1. International Wound Infection Institute (IWII) Wound Infection in Clinical Practice. Wounds International 2022.

Simplifying product choice

Wound Infection Product Selection Guide



Step 1: Assess

Assess the wound using the Wound Infection pathway

Step 2: Prepare

Prepare the wound for healing.
Use Alprep® Pad or follow local guidance.

Step 3: Treat

Treat the wound in accordance with underlying aetiology and specific wound treatment objectives

Alprep® Pad



Superficial



Biatain® Silicone Ag
or



Biatain® Ag Non-Adhesive

0-2cm in depth*



Biatain® Silicone Ag
or



Biatain® Ag Non-Adhesive

>2cm in depth



Biatain® Alginate Ag
+



Biatain® Silicone or
Biatain® Non-Adhesive

Undermining/Tunneling



Biatain® Alginate Ag
+



Biatain® Silicone or
Biatain® Non-Adhesive

*Conformability may vary across product design

This information is for general guidance only and should not replace clinical judgement. If you are unsure, seek TVN advice. For further product information please refer to the Instructions For Use packaged with the product.

The Coloplast logo is a registered trademark of Coloplast A/S. © 2024 All rights reserved Coloplast A/S

CM777N / PM-30169

